

A rapid diagnostic test for the detection of *Clostridium difficile* GDH, Toxin A and Toxin B antigens in human feces samples. For *in vitro* professional use only.

INTENDED USE

The *Clostridium difficile* GDH +Toxin A +Toxin B Combo Rapid Test Cassette (Feces) is a rapid chromatographic immunoassay for the qualitative detection of *Clostridium difficile* GDH, Toxin A and Toxin B antigens in the human feces specimen.

SUMMARY

Clostridium difficile is an anaerobic bacteria acting as an opportunistic pathogen: it grows in the intestine when the normal flora has been altered by treatment with antibiotics.^{1,2,3} Toxinogenic strains of *Clostridium difficile* cause infections from mild-diarrhea to pseudomembranous colitis, potentially leading to death.⁴ Disease is caused by two toxins produced by toxinogenic strains of *C. difficile*: Toxin A (tissue-damaging enterotoxin) and Toxin B (cytotoxin). Some strains produce both toxins A and B, some others produce Toxin B only. The potential role of a third (binary) toxin in pathogenicity is still debated.⁴ The use of Glutamate Dehydrogenase (GDH) as an antigen marker of *C. difficile* proliferation has been shown to be very effective because all strains produce high amount of this enzyme.^{5,6} *Clostridium difficile* GDH+ Toxin A +Toxin B Combo Rapid Test Cassette allows the detection of GDH, Toxin A and Toxin B specific to *C. difficile* in fecal specimen.

PRINCIPLE

Clostridium difficile Rapid Test Cassette detects three distinct antigens in fecal specimens for *C. difficile*, viz., GDH, Toxin A and Toxin B on three different test strips in a single test cassette, thus simultaneously detecting three antigens specific of *Clostridium difficile*.

For *C. difficile*-specific GDH Testing

The membrane is precoated with anti-*C.diff* GDH antibody on the test line region. During testing, the specimen reacts with the particle coated with anti-*C.diff* GDH antibody. The mixture migrates upward on the membrane chromatographically by capillary action to react with anti-*C.diff* GDH antibody on the membrane and generate a colored line.

For *C. difficile*-specific Toxin A Testing

The membrane is precoated with anti-*C.diff* Toxin A antibody on the test line region. During testing, the specimen reacts with the particle coated with anti-*C.diff* Toxin A antibody. The mixture migrates upward on the membrane chromatographically by capillary action to react with anti-*C.diff* Toxin A antibody on the membrane and generate a colored line. The presence of this colored line in the test line region indicates a positive result, while its absence indicates a negative result.

For *C. difficile*-specific Toxin B Testing

The membrane is precoated with anti-*C.diff* Toxin B antibody on the test line region. During testing, the specimen reacts with the particle coated with anti-*C.diff* Toxin B antibody. The mixture migrates upward on the membrane chromatographically by capillary action to react with anti-*C.diff* Toxin B antibody on the membrane and generate a colored line. The presence of this colored line in the test line region indicates a positive result, while its absence indicates a negative result.

To serve as a procedural control, a colored line will always appear in the control line region of all the three test strips, indicating that the proper volume of specimen has been added and membrane wicking has occurred.

REAGENTS

The test cassette contains anti-*Clostridium difficile* GDH, anti-*Clostridium difficile* Toxin A and anti-*Clostridium difficile* Toxin B antibody coated particles anti-*Clostridium difficile* GDH, anti-*Clostridium difficile* Toxin A and anti-*Clostridium difficile* Toxin B coated on the membrane.

PRECAUTIONS

- For professional *in vitro* diagnostic use only. Do not use after expiration date.
- The test should remain in the sealed pouch until use.
- Do not eat, drink or smoke in the area where the specimens or kits are handled.
- Handle all specimens as if they contain infectious agents. Observe established precautions against microbiological hazards throughout all procedures and follow the standard procedures for proper disposal of specimens.
- Wear protective clothing such as laboratory coats, disposable gloves and eye protection when specimens are assayed.
- The used test should be discarded according to local regulations.
- Humidity and temperature can adversely affect results.

STORAGE AND STABILITY

Store as packaged at room temperature or refrigerated (2-30°C). The test is stable through the expiration date printed on the sealed pouch. The test must remain in the sealed pouch until use. **DO NOT FREEZE**. Do not use beyond the expiration date.

SPECIMEN COLLECTION AND PREPARATION

The stool specimens must be tested as soon as possible after collection. If necessary, original feces specimen could be stored at 2-8°C for 3 days or -20°C for longer periods of time; extracted specimen in buffer could be stored at 2-8°C for 1 week or -20°C for longer periods of time.

Make sure that the specimens are not treated with solutions containing formaldehyde or its derivatives.

MATERIAL

Materials provided

- Test Cassettes
- Droppers
- Package Insert
- Specimen Collection Tubes with Buffer
- Materials required but not provided
- Stool Containers
- Timer
- Centrifuge

PROCEDURE


Allow the test, specimen and collection buffer to equilibrate to room temperature (15-30°C) prior to testing.

- To collect fecal specimens:

Collect sufficient quantity of feces (1-2mL or 1-2g) in a clean, dry specimen collection container to obtain enough antigens (if present). Best results will be obtained if the assay is performed within 6 hours after collection. Specimen collected may be stored for 3 days at 2-8°C if not tested within 6 hours. For long term storage, specimens should be kept below -20°C.
 - To process fecal specimens:
 - For **Solid Specimens**:

Unscrew the cap of the specimen collection tube, then randomly stab the specimen collection applicator into the fecal specimen at least 3 different sites to collect approximately 50 mg of feces (equivalent to 1/4 of a pea). Do not scoop the fecal specimen.
 - For **Liquid Specimens**:

Hold the dropper vertically, aspirate fecal specimens, and then transfer 2 drops of the liquid specimen (approximately 80 µL) into the specimen collection tube containing the extraction buffer. Tighten the cap onto the specimen collection tube, and then shake the specimen collection tube vigorously to mix the specimen and the extraction buffer. Leave the collection tube for reaction for 2 minutes.
 - Bring the pouch to room temperature before opening it. Remove the test cassette from the foil pouch and use it as soon as possible. Best results will be obtained if the test is performed immediately after opening the foil pouch.
 - Hold the specimen collection tube upright and unscrew the tip of the specimen collection tube. Invert the specimen collection tube and transfer 3 full drops of the extracted specimen (approximately 120 µL) to each of the specimen well(S) of the test cassette, then start the timer. Avoid trapping air bubbles in the specimen well (S). See illustration.
 - Read the results at 10 minutes after dispensing the specimen. Do not read results after 20 minutes.
- Note:** If the specimen does not migrate (presence of particles), centrifuge the diluted sample contained in the extraction buffer vial. Collect 120µL of supernatant, dispense into the specimen well (S). Start the timer and continue from step 5 onwards in the above instructions for use.

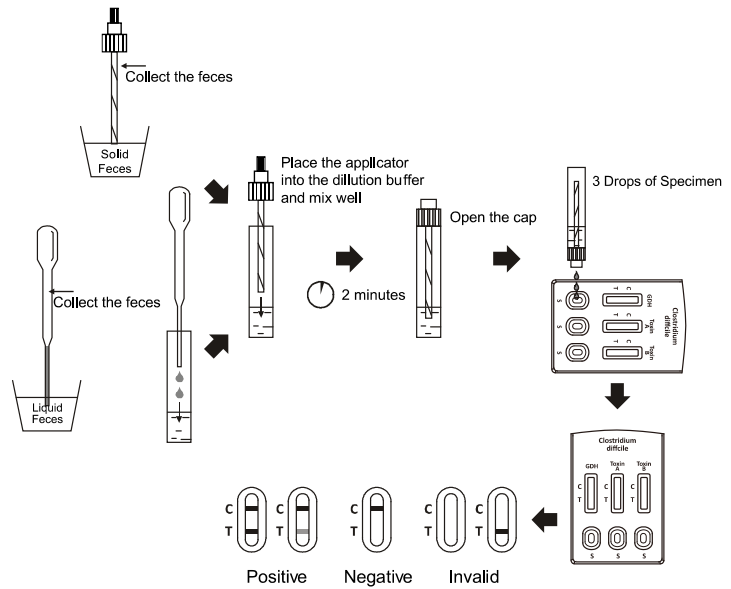

INTERPRETING RESULTS

The test results appear in three different test windows respectively for GDH, Toxin A or Toxin B. The interpretation criteria remain the same for positivity or negativity for specific antigens under tests as per indication of the respective Test window. The results are to be interpreted as follows:

POSITIVE: *Two colored lines appear. One colored line should be in the control line region (C) and another apparent colored line should be in the test line region (T).

*NOTE: The intensity of the color in the test line region (T) will vary depending on the concentration of *Clostridium difficile* antigens present in the specimen. Therefore, any shade of color in the test line region (T) should be considered positive.

NEGATIVE: One colored line appears in the control line region (C). No line appears in the test line region (T).

INVALID: Control line (C) fails to appear. Insufficient specimen volume or incorrect procedural techniques are the most likely reasons for control line failure. Review the procedure and repeat the test with a new test. If the problem persists, discontinue using the test kit immediately and contact your local distributor.

QUALITY CONTROL

An internal procedural control is included in the test. A colored line appearing in the control line region (C) is an internal procedural control. It confirms sufficient specimen volume, adequate membrane wicking and correct procedural technique.

Control standards are not supplied with this kit; however, it is recommended that positive and negative controls be tested as a good laboratory practice to confirm the test procedure and to verify proper test performance.

LIMITATION

- The *Clostridium difficile* GDH +Toxin A +Toxin B Combo Rapid Test Cassette (Feces) is for *in vitro* diagnostic use only.
- The test is qualitative and cannot predict the quantity of antigens present in the sample. Clinical presentation and other test results must be taken into consideration to establish diagnosis.
- A positive test does not rule out the possibility that other pathogens may be present.

PERFORMANCE

Detection Limit

Detection limit values of *Clostridium difficile* GDH+Toxin A+Toxin B Combo Rapid Test Cassette was 1ng/mL for GDH, 2ng/mL for Toxin A and 7ng/mL for Toxin B.

Sensitivity - Specificity

Clostridium difficile GDH Results

Method	Results	Other Rapid Test		Total Results
		Positive	Negative	
<i>Clostridium difficile</i> GDH +Toxin A +Toxin B Combo Rapid Test Cassette (Feces)	Positive	116	8	124
	Negative	6	170	176
Total Results		122	178	300

Relative Sensitivity: 95.1% (95%CI:*89.6%-98.2%)

*Confidence Intervals

Relative Specificity: 95.5% (95%CI:*91.3%-98.0%)

Relative Accuracy: 95.3% (95%CI:*92.3%-97.4%)

Clostridium difficile Toxin A Results

Method	Results	Other Rapid Test		Total Results
		Positive	Negative	
<i>Clostridium difficile</i> GDH +Toxin A +Toxin B Combo Rapid Test Cassette (Feces)	Positive	115	5	120
	Negative	7	173	180
Total Results		122	178	300

Relative Sensitivity: 94.3% (95%CI:*88.5%-97.7%)

*Confidence Intervals

Relative Specificity: 97.2% (95%CI:*93.6%-99.1%)

Relative Accuracy: 96.0% (95%CI:*93.1%-97.9%)

Clostridium difficile Toxin B Results

Method	Results	Other Rapid Test		Total Results
		Positive	Negative	
<i>Clostridium difficile</i> GDH +Toxin A +Toxin B Combo Rapid Test Cassette (Feces)	Positive	112	6	118
	Negative	10	172	182
Total Results		122	178	300

Relative Sensitivity: 91.8% (95%CI:*85.4%-96.0%)

*Confidence Intervals

Relative Specificity: 96.6% (95%CI:*92.8%-98.8%)

Relative Accuracy: 94.7% (95%CI:*91.5%-96.9%)

Precision

Intra-assay and inter-assay

To check intra-batch accuracy (repeatability), the same positive samples and a buffer solution were processed 3 times on test kits of the same batch number in the same experimental conditions. All observed results were confirmed as expected.

To check inter-batch accuracy (reproducibility), same samples (positive and buffer) were processed on test kits from three different batches. All results were confirmed as expected.

Cross Reactivity

An evaluation was performed to determine the cross reactivity of *Clostridium difficile* GDH +Toxin A +Toxin B Combo Rapid Test Cassette (Feces). No cross reactivity against gastrointestinal pathogens occasionally present as following:

<i>Campylobacter coli</i>	<i>Salmonella enteritidis</i>	<i>Shigella dysenteriae</i>
<i>Campylobacter jejuni</i>	<i>Salmonella paratyphi</i>	<i>Shigella flexneri</i>
<i>E.coli</i> O157:H7	<i>Salmonella typhi</i>	<i>Shigella sonnei</i>
<i>H.pylori</i>	<i>Salmonella typhimurium</i>	<i>Staphylococcus aureus</i>
<i>Listeria monocytogenes</i>	<i>Shigella boydii</i>	<i>Yersinia enterocolitica</i>

Interfering Substances












The following potentially Interfering Substances were added to *Clostridium difficile* GDH+Toxin A+Toxin B negative and positive specimens.

Ascorbic acid: 20mg/dL	Oxalic acid: 60mg/dL	Bilirubin: 100mg/dL
Uric acid: 60mg/dL	Aspirin: 20mg/dL	Urea: 2000mg/dL
Glucose: 2000mg/dL	Caffeine: 40mg/dL	Albumin: 2000mg/dL

BIBLIOGRAPHIC REFERENCES

1. Ramadass Balamurugan, V. Balaji and Balakrishnan S. Ramakrishna: *Estimation of faecal carriage of Clostridium difficile in patients with ulcerative colitis using real time polymerase chain reaction*, Indian Journal of Medical Research, p.472-477, May 2008
2. E. J. Kuijper, B. Coignard and P. Till: *Emergence of Clostridium difficile-associated disease in North America and Europe*, Review Clinical Microbiology and Infections, 12 suppl6, p. 2-18, Oct. 2006
3. Leyerly D.M., H.C. Krivan and D.T. Wilkins: *Clostridium difficile: its disease and toxins*. Clinical Microbiology Reviews, p. 1-18, Jan. 1988
4. Ramsey L. et al: *Fulminant Clostridium difficile: an underappreciated and increasing cause of death and complications*, Annals of Surgery 235 (3) p. 363-372: Mar. 2002
5. Wren MW., Kinson R., Sivapalan M., Shemko M., Shetty NR.: *Detection of Clostridium difficile infection: a suggested laboratory diagnostic algorithm*, British Journal of Biomedical Sciences, 66(4) p. 175-179, 2009.
6. Willis DH. And JA Kraft: *Confirmation that the latex-reactive protein of Clostridium difficile is a Glutamate Dehydrogenase*. Journal of clinical microbiology, 30, p. 1363-1364, May 1992

Index of Symbols

	Consult Instructions For Use		Tests per kit		Authorized Representative
	For <i>in vitro</i> diagnostic use only		Use by		Do not reuse
	Store between 2-30°C		Lot Number		Catalog #
	Do not use if package is damaged		Manufacturer		

ACRO BIOTECH, Inc.
 4650 Arrow Highway,
 Suite D-6 Montclair, CA 91763, U.S.A.
 Tel: +1 (909) 541-5085 www.acrobiotech.com




 MedNet EC-REP GmbH
 Borkstrasse 10
 48163 Muenster
 Germany

Number: 146301001
 Revision date: 2023-01-28